Adapting to Pentax Immersible GI Endoscopes**

With Push In Air/Water & Suction Valves

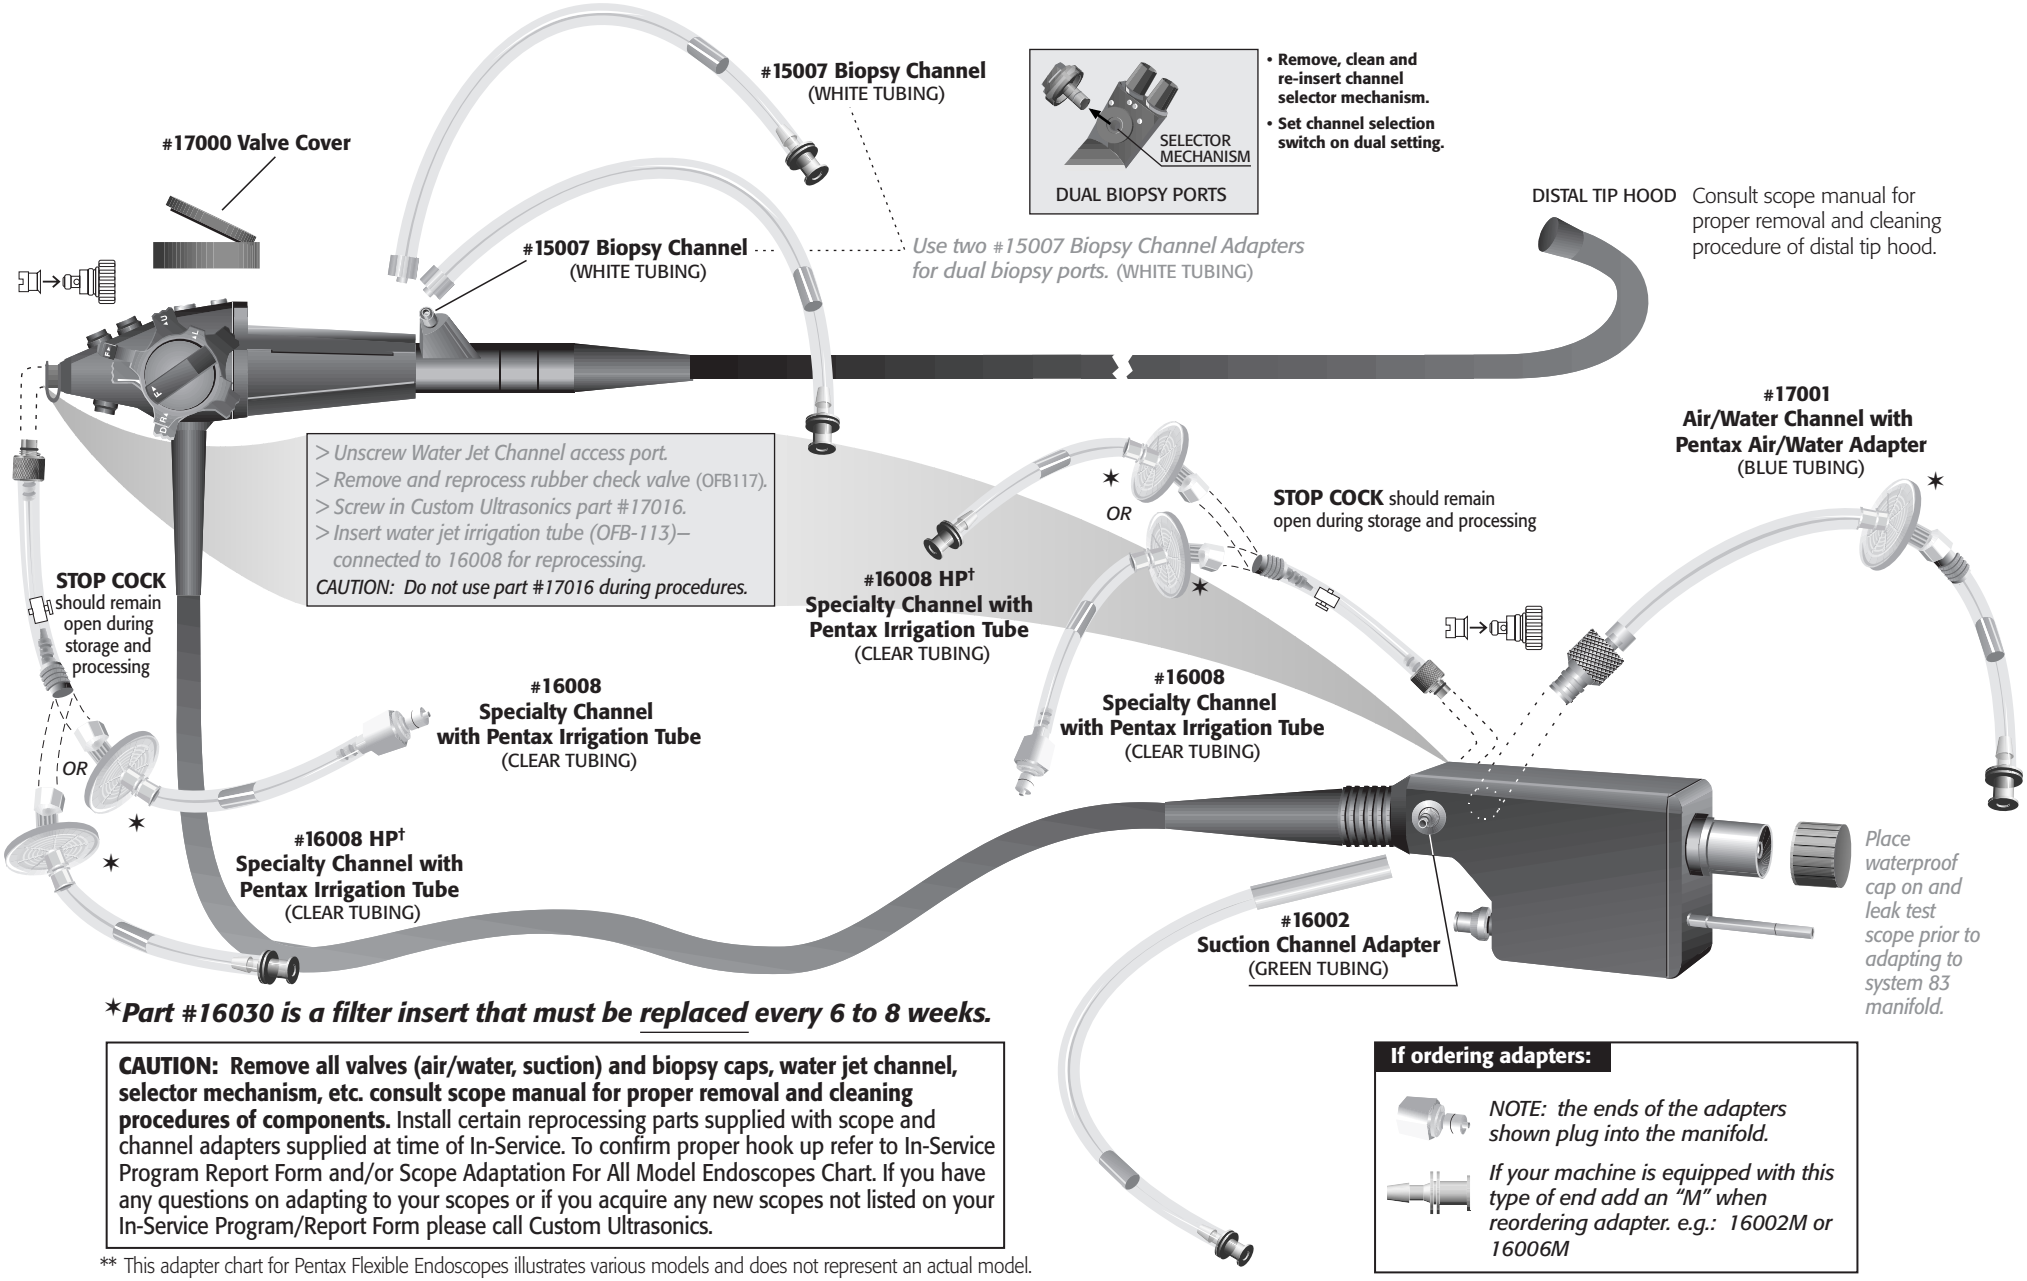

✶***Part #16030 is a filter insert that must be replaced every 6 to 8 weeks.***

CAUTION: Remove all valves (air/water, suction) and biopsy caps, water jet channel, selector mechanism, etc. consult scope manual for proper removal and cleaning procedures of components. Install certain reprocessing parts supplied with scope and channel adapters supplied at time of In-Service. To confirm proper hook up refer to In-Service Program Report Form and/or Scope Adaptation For All Model Endoscopes Chart. If you have any questions on adapting to your scopes or if you acquire any new scopes not listed on your In-Service Program/Report Form please call Custom Ultrasonics.

If ordering adapters:

NOTE: the ends of the adapters shown plug into the manifold.

If your machine is equipped with this type of end add an "M" when reordering adapter. e.g.: 16002M or 16006M

** This adapter chart for Pentax Flexible Endoscopes illustrates various models and does not represent an actual model.

† For machines that are equipped with High Pressure Ports use #16008 HP Specialty Channel.

Custom Ultrasonics INCORPORATED

P.O. Box 850 Buckingham, PA 18912 (215) 364-1477 FAX (215) 364-7674 www.customultrasonics.com

JUNE2004-PEN(1)